



EASTMAN

**Redefining the balance
between processibility
and chemical resistance**

A new-generation copolyester

Eastman **TRITAN™**
copolyester

Transforming the potential for medical-grade polymers

Eastman has supplied a wide range of materials for the medical market for more than 65 years. Today, the company is committed to the long-term needs of the medical industry and is a reliable supplier of innovative medical-grade polymers and technical support for a variety of applications, including molded medical devices.

Now, we're even better prepared to provide a "total solutions" approach to the needs of the medical industry because of the addition of Eastman Tritan™ copolyester to our polymers portfolio.

Tritan builds on the rich heritage of other successful Eastman brands, including DuraStar™ polymer, Eastar™ copolyester, and Tenite™ cellulose. Like our traditional polymers, Tritan provides outstanding lipid and chemical resistance and is free of bisphenol A (BPA) and halogens. It also offers greater toughness, heat resistance, and processibility than heritage copolyesters.

This unique combination of properties allows Tritan to satisfy a set of customer needs that have not been met by other Eastman polymers—or by many other polymers available to the medical industry today.



When innovation exceeds expectations

Eastman Tritan™ copolyester MX711 is an innovative, clear medical-grade polymer that delivers a unique balance of design, processing, and physical properties for medical devices.

- For applications that demand superior chemical resistance, clarity, and hydrolytic stability, Tritan provides the advantages of a copolyester.
- For clear applications that demand easier processibility and greater durability, Tritan offers performance that is comparable, or in many cases superior, to other medical-grade polymers.

Expect a balance of important advantages

Tritan MX711 combines design, processing, and physical properties that are most important in medical devices.

Processibility

The innovative chemistry of Tritan provides enhanced heat resistance as well as:

- Easier processing
- Faster cycle times
- Molded part shrinkage similar to polycarbonate (PC)

For medical-grade applications requiring thin walls or intricate design, Tritan is available in a high-flow product, Eastman Tritan™ copolyester MX731 (see page 9).

Chemical resistance

Tritan offers excellent resistance to the effects of exposure to common substances found in the medical environment that can lead to environmental stress cracking and functional deterioration:

- Blood and lipids
- Chemical agents like isopropyl alcohol (IPA), disinfectants, and bonding solvents

Toughness

Risk is reduced for manufacturers through:

- Excellent toughness
- Fewer broken parts, reduced part failure, and less waste
- Greater customer satisfaction

Hydrolytic stability

Tritan has outstanding hydrolytic stability, so parts made from this innovative polymer are unlikely to deteriorate when exposed to heat, humidity, and chemical agents.

Compatibility with sterilization methods

Reliable long-term clarity, color stability, and retention of functional integrity following sterilization by:

- Gamma irradiation
- Electron beam (e-beam) irradiation
- Ethylene oxide (EtO) gas



Clarity

Tritan MX711 provides glasslike transparency that conveys safety, quality, and peace of mind for both healthcare professionals and patients.

BPA free

Like all Eastman copolyesters and cellulose, Tritan is made without BPA or halogens.

Secondary operations and assembly

Tritan MX711 is compatible with a wide variety of manufacturing operations and techniques, including:

- Solvent and adhesive bonding
- Ultrasonic welding
- Laser welding
- Cold swaging

Heat resistance

Enhanced heat resistance relative to heritage copolyesters:

- Slower physical aging
- Reduced creep

Explore a wide range of applications

Tritan is well-suited for medical-device applications that demand superior chemical resistance, clarity, and hydrolytic stability, including:

- IV system components
- Blood therapy devices

The following pages show how Tritan's advantages have been validated. Let us show you how this innovative polymer can deliver performance and peace of mind in your medical-device applications.




When innovation meets validation

Eastman is committed to providing information about its medical-grade polymers. The Eastman Medical Applications Development Team has tested Eastman Tritan™ copolyester MX711 under rigorous conditions against other popular polymers for the properties that are most important for high-quality medical devices. More trial results for this innovative polymer are available on request.

Chemical resistance



Excellent resistance against lipids, IPA, disinfecting agents, and bonding solvents is a respected legacy for Eastman copolyesters; Tritan MX711 continues this tradition. In this trial, the chemical resistance of Tritan MX711 was compared with high-flow PC, lipid-resistant PC, and impact-modified acrylic. Eastar™ copolyester MN006 natural also was compared as a benchmark.

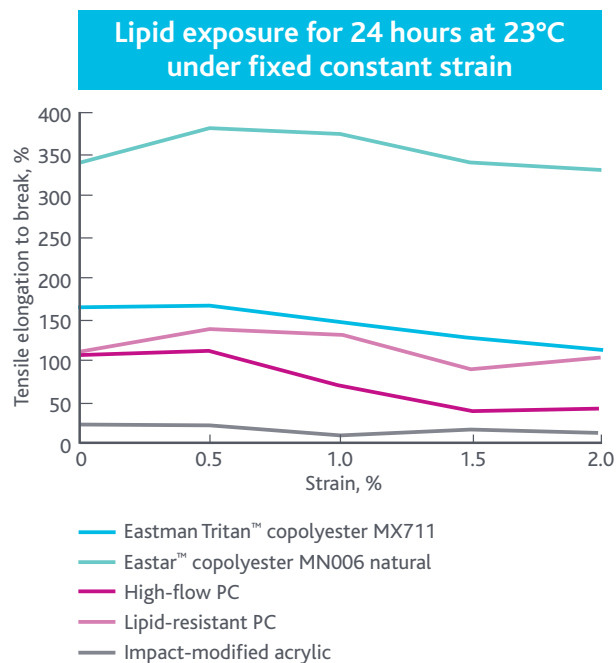

Toughness

Tritan MX711 delivers exceptional toughness. It offers impact and shatter resistance that is comparable to PC. In this trial, Tritan MX711 was tested according to ASTM D256 Notched Izod Impact at 23°C.


Eastar™ copolyester MN006 natural as well as a medical-grade acrylic and PC were tested for comparison. Two thicknesses were evaluated, the standard 1/8 inch as well as 1/4 inch. Tritan MX711 maintains high-impact strength at both thicknesses.

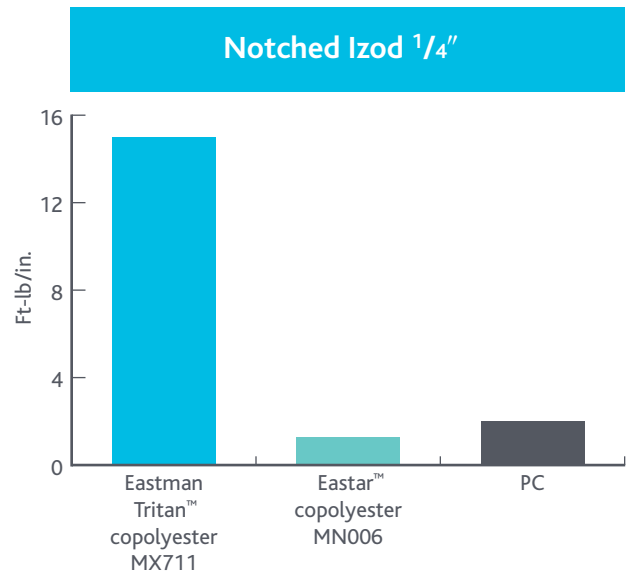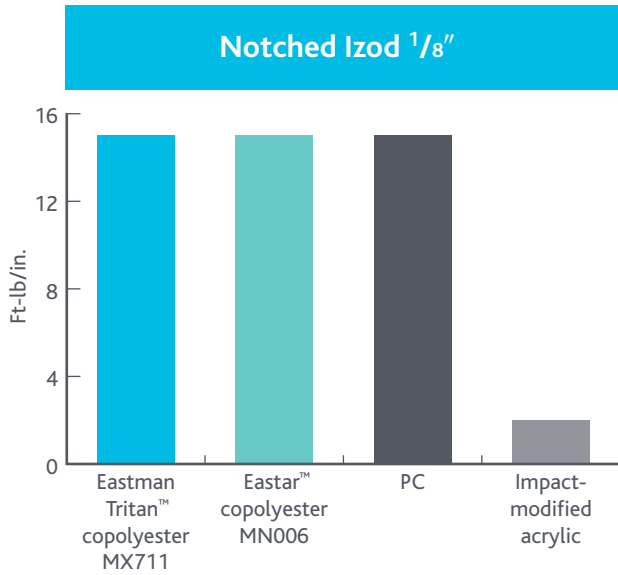

Hydrolytic stability

Tritan demonstrates excellent stability against high humidity, moderate heat, and aggressive chemical environments.

Samples were strained to varying degrees and exposed to typical residential dishwasher conditions. Tritan shows no cracking or crazing even after hundreds of wash cycles; PC fails quickly when exposed to this environment.


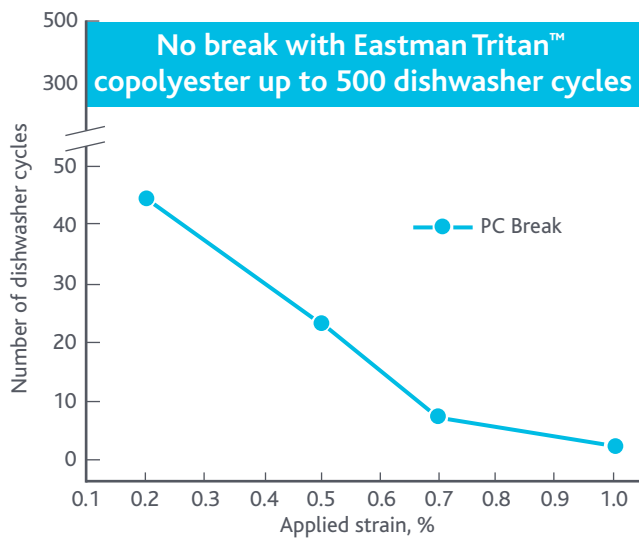


Sterilization

Both e-beam and gamma irradiation are known to change polymers subjected to these processes—changes which can impact color and overall aesthetics, color-coding options, and even functional integrity. Tritan MX711 was compared with PC, acrylic, DuraStar MN611 natural, and Eastar MN006.

For applications involving e-beam, gamma, EtO, or other low-temperature sterilization processes, Tritan MX711 gives outstanding, reliable performance.

Eastman provides a “total solutions” approach for medical-device manufacturers, leveraging years of experience with innovative materials, such as Tritan, to deliver the best solution for your needs.

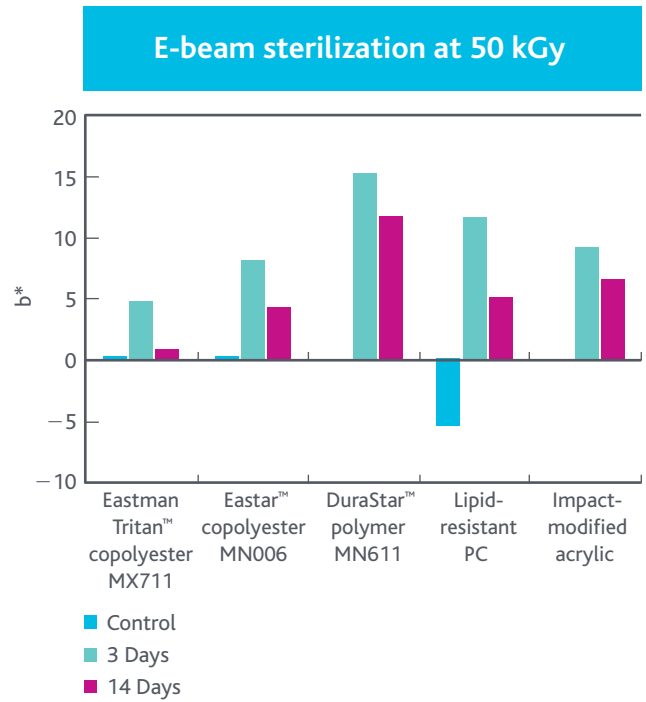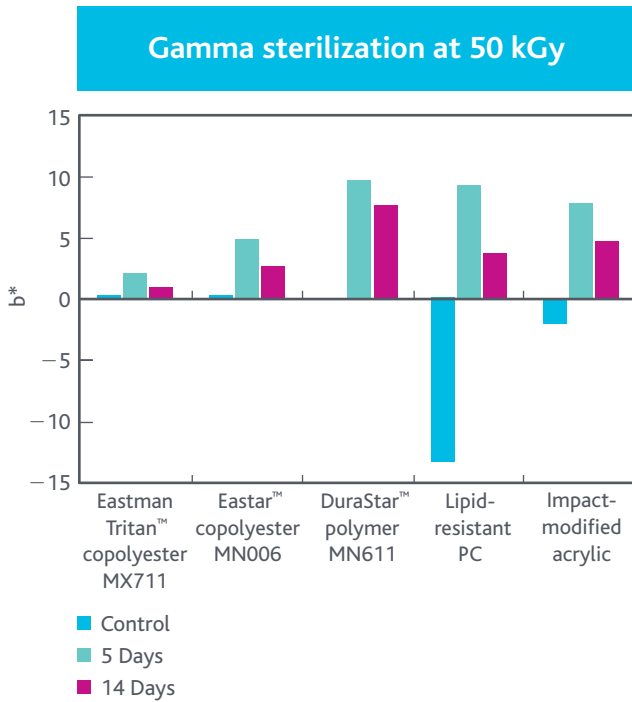

Committed to making a material difference

As a committed medical polymer solutions provider, Eastman can leverage its industry understanding—along with extensive design, engineering, and manufacturing expertise—to help customers develop products, bring them to market quickly, and follow through with strong technical support.

Eastman provides a wide variety of polymer solutions through its family of product offerings. Let our experienced professionals help select the right balance of properties for your applications.

Comparison of medical-grade polymers

Material	Desired property					Comments
	Higher heat resistance	Toughness	Lipid resistance	Solvent bonding	Faster injection molding cycles	
Eastman Tritan™ copolyester MX711						Superior clarity after sterilization; BPA free; hydrolytic stability
DuraStar™ polymer						BPA free
Eastar™ copolyester						Superior clarity after sterilization; BPA free
Tenite™ cellulosics						BPA free
PC ^a						PC typically requires annealing at faster mold cycles to improve chemical resistance
Impact-modified acrylic ^b						BPA free

Best
 Good
 Average
 Fair
 Poor

^aPC represents high-flow PC.

^bToughened acrylic represents impact-modified acrylic.

Eastman Tritan™ copolyester MX731—a high-flow, medical-grade product

For molding parts such as cannulae, with long thin walls or deep cavitation sections, Tritan MX731 provides a practical solution.

Tritan MX731 provides the benefits of high-flow lengths while maintaining the polymer’s other important benefits:

- Chemical resistance
- Toughness
- Clarity
- Color stability

When innovation matches application


With current trends driving an increased need for simple, robust, and reliable medical devices, a partner with Eastman's experience can be invaluable for matching technology to your needs.


With more than 20 years of experience, the Eastman Medical Applications Development Team has assisted customers in the development of component medical parts that meet the functional and aesthetic requirements of the medical industry.

From mold design to end-use performance, medical-device manufacturers can count on Eastman for extensive technical support, including:

- Polymer selection
- Part design
- Tooling
- Mold-filling simulation
- Secondary operations

The Eastman Medical Applications Development Team works with customers at all stages of the process—beginning early in the design and specification stage to optimize development of the medical device. With the assurance that Tritan MX711 and high-flow MX731 are matched with the proper part design, suitable mold design, and recommended processing parameters, designers and molders can achieve the most efficient manufacturing of high-performance, reliable medical devices.

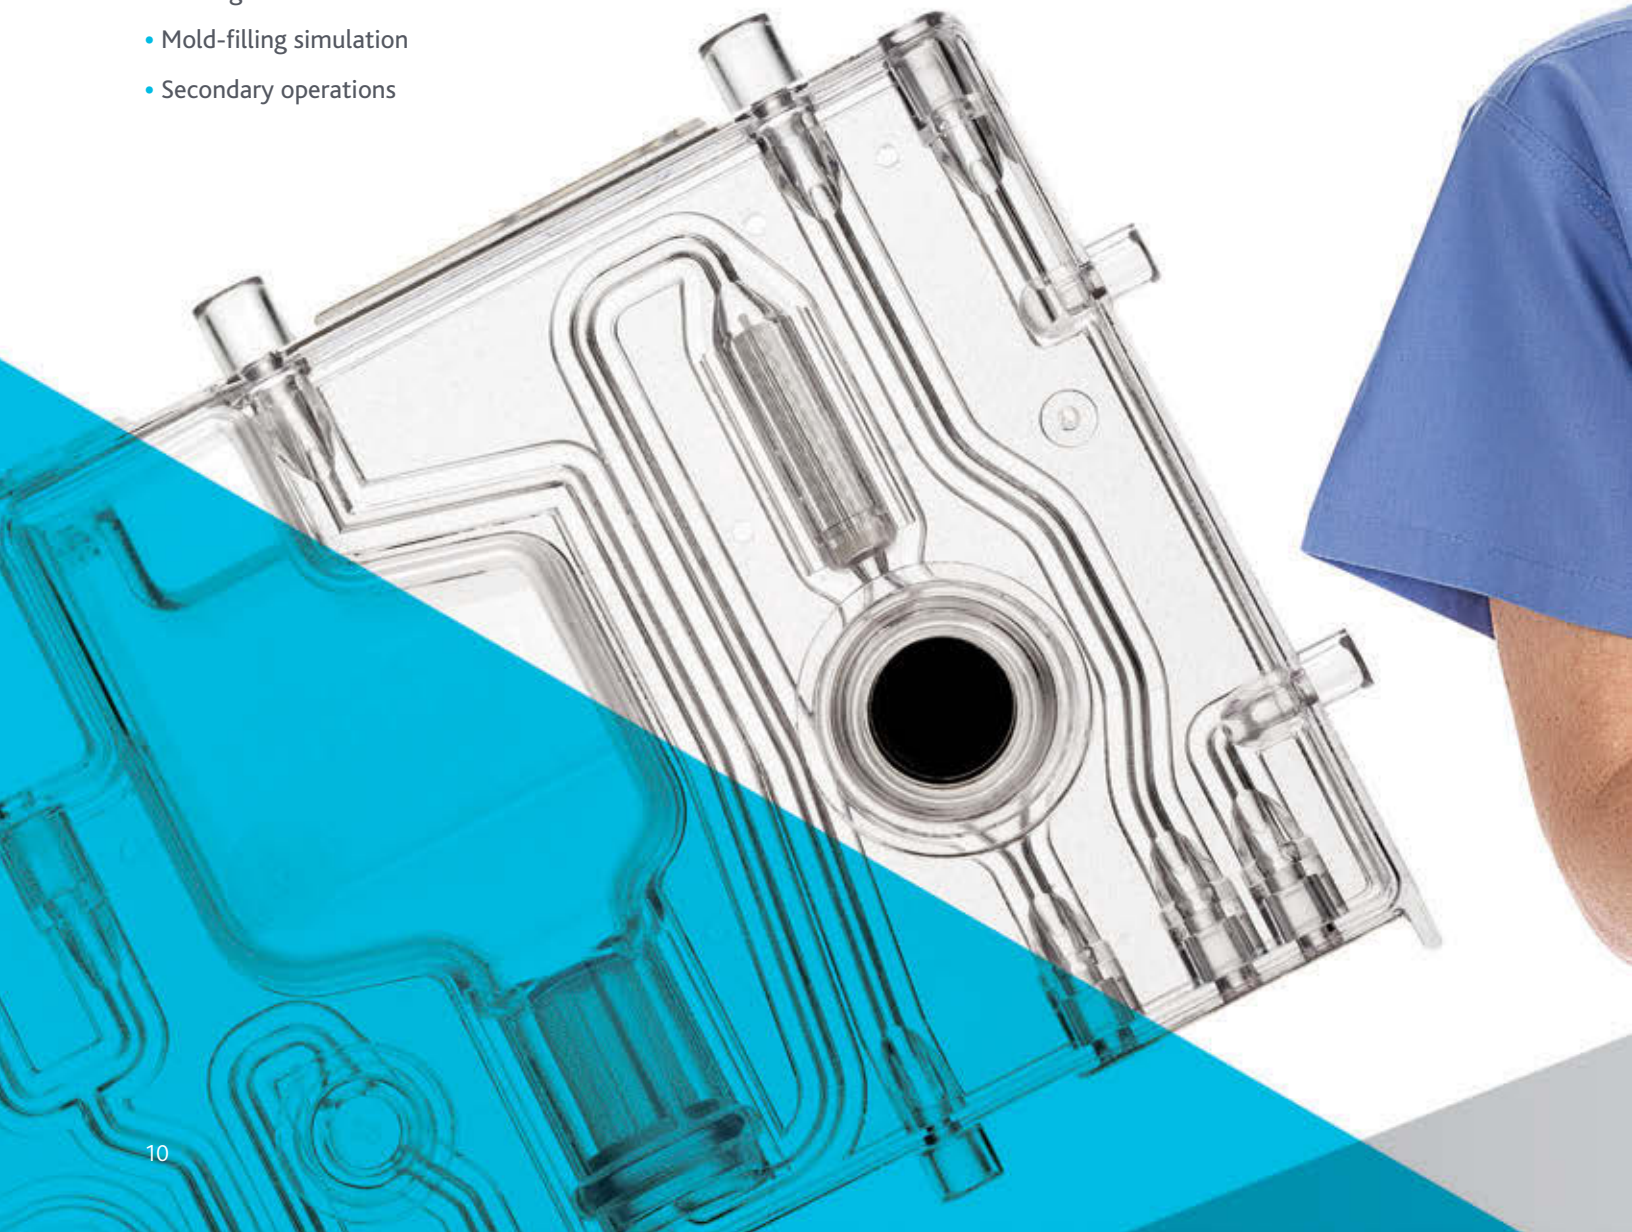

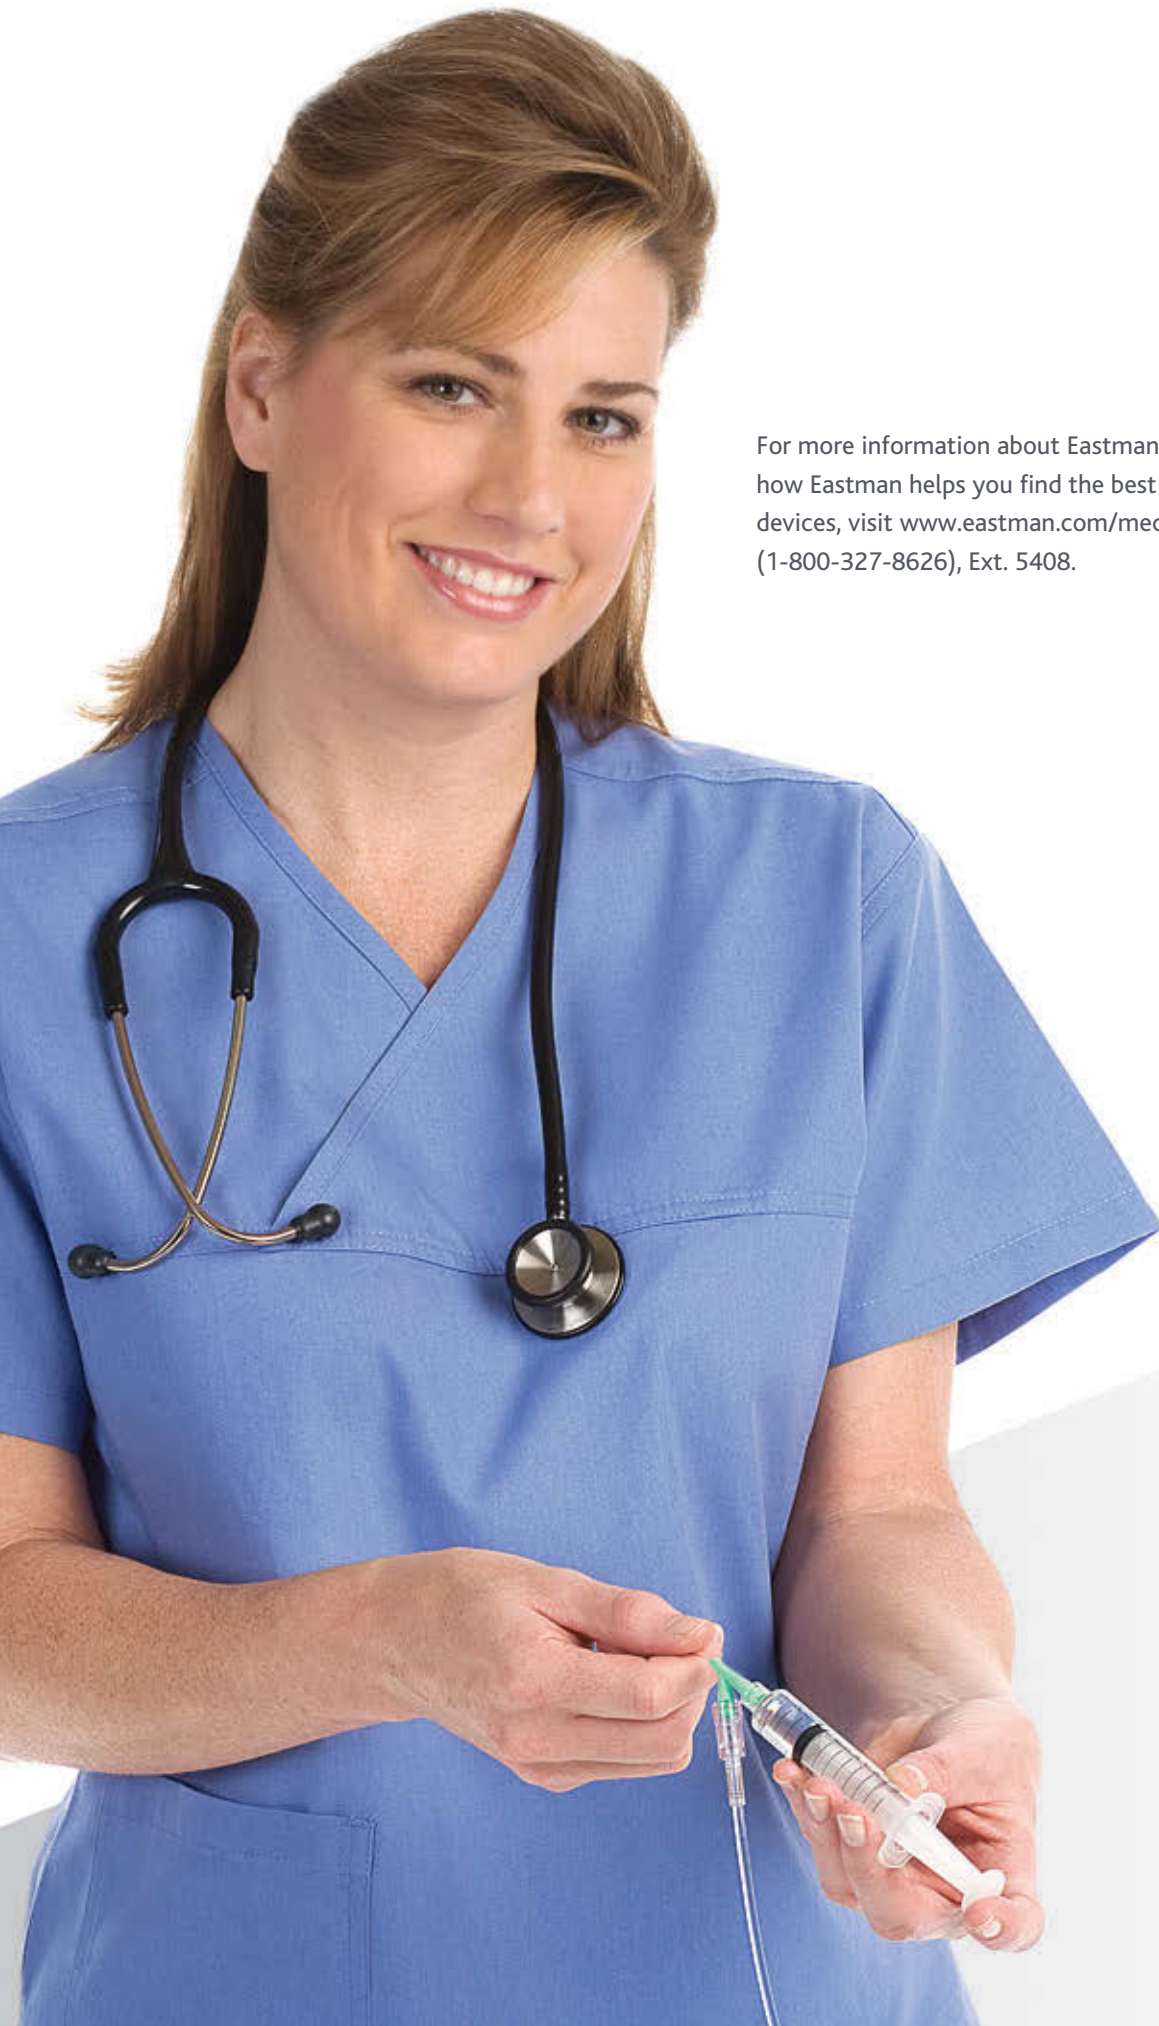

For more information about Eastman Tritan™ copolyester and how Eastman helps you find the best solutions for your medical devices, visit www.eastman.com/medical or call 1-800-EASTMAN (1-800-327-8626), Ext. 5408.



The results of insight™

Eastman Chemical Company Corporate Headquarters

P.O. Box 431
Kingsport, TN 37662-5280 U.S.A.

Telephone:
U.S.A. and Canada, 800-EASTMAN (800-327-8626)
Other Locations, (1) 423-229-2000
Fax: (1) 423-229-1193

Eastman Chemical Latin America

9155 South Dadeland Blvd.
Suite 1116
Miami, FL 33156 U.S.A.

Telephone: (1) 305-671-2800
Fax: (1) 305-671-2805

Eastman Chemical B.V.

Fascinatio Boulevard 602-614
2909 VA Capelle aan den IJssel
The Netherlands

Telephone: (31) 10 2402 111
Fax: (31) 10 2402 100

Eastman (Shanghai) Chemical Commercial Company, Ltd.

Building C, No. 399 Shengxia Road,
Pudong New District
201210, Shanghai, P.R. China

Telephone: (86) 21 6120-8700
Fax: (86) 21 5027-9229

Eastman Chemical Japan Ltd.

MetLife Aoyama Building 5F
2-11-16 Minami Aoyama
Minato-ku, Tokyo 107-0062 Japan

Telephone: (81) 3-3475-9510
Fax: (81) 3-3475-9515

Eastman Chemical Asia Pacific Pte. Ltd.

9 North Buona Vista Drive
#05-01 The Metropolis Tower 1
Singapore 138588

Telephone: (65) 6831-3100
Fax: (65) 6732-4930

www.eastman.com

Eastman Tritan™ copolyester is not approved for implantable devices.

Safety Data Sheets providing safety precautions that should be observed when handling and storing Eastman products are available online or by request. You should obtain and review the available material safety information before handling any of these products. If any materials mentioned are not Eastman products, appropriate industrial hygiene and other safety precautions recommended by their manufacturers should be observed.

It is the responsibility of the medical device manufacturer ("Manufacturer") to determine the suitability of all component parts and raw materials, including any Eastman product, used in its final product to ensure safety and compliance with requirements of the United States Food and Drug Administration (FDA) or other international regulatory agencies.

Eastman products have not been designed for nor are they promoted for end uses that would be categorized either by the United States FDA or by the International Standards Organization (ISO) as implant devices. Eastman products are not intended for use in the following applications: (1) in any bodily implant applications for greater than 30 days, based on FDA-Modified ISO-10993, Part 1, "Biological Evaluation of Medical Devices" tests (including any cosmetic, reconstructive, or reproductive implant applications); (2) in any cardiac prosthetic device application, regardless of the length of time involved, including, without limitation, pacemaker leads and devices, artificial hearts, heart valves, intra-aortic balloons and control systems, and ventricular bypass assisted devices; or (3) as any critical component in any medical device that supports or sustains human life.

For manufacturers of medical devices, biological evaluation of medical devices is performed to determine the potential toxicity resulting from contact of the component materials of the device with the body. The ranges of tests under FDA-Modified ISO-10993, Part 1, "Biological Evaluation of Medical Devices" include cytotoxicity, sensitization, irritation or intracutaneous reactivity, systemic toxicity (acute), subchronic toxicity (subacute), implantation, and hemocompatibility. For Eastman products offered for the medical market, limited testing information is available on request. The Manufacturer of the medical device is responsible for the biological evaluation of the finished medical device.

The suitability of an Eastman product in a given end-use environment is dependent on various conditions including, without limitation, chemical compatibility, temperature, part design, sterilization method, residual stresses, and external loads. It is the responsibility of the Manufacturer to evaluate its final product under actual end-use requirements and to adequately advise and warn purchasers and users thereof.

© 2014 Eastman Chemical Company. Eastman, DuraStar, Eastar, Tenite, The results of insight, and Tritan are trademarks of Eastman Chemical Company.